



A DIRECT HEALTHCARE GROUP COMPANY

# Bure Rise & Go DB

## Technical Manual





# Bure Rise & Go DB

The Bure Rise & Go is a cost-effective walker enhanced with a patented power rise function. Thanks to the electric power rise function, Bure Rise & Go acts as a combined stand-up, mobility and walking aid all in a single product. Rise & Go is now also available with electric walking frame widening. Flexible widening combined with the lower height above the walking frame enhances versatility regardless of the patient's situation in hospital or at home.

## Contents

|                                       |    |
|---------------------------------------|----|
| 1. Replacement parts list             | 04 |
| 2. Accessories                        | 04 |
| 3. Electrical system – Technical data | 06 |
| 4. Remote Control Plus                | 06 |
| 5. Control box wiring                 | 07 |
| 6. Battery charging                   | 07 |
| 7. LED on controlbox and battery      | 07 |
| 8. Maintenance                        | 08 |
| 9. General safety/maintenance advice  | 09 |
| 10. ID label                          | 09 |
| 11. Recycling/Scrapping               | 10 |
| 12. Warranty                          | 10 |
| 13. Technical specifications          | 10 |

## 1. Replacement parts list


|           |                    |  |           |                            |  |
|-----------|--------------------|--|-----------|----------------------------|--|
| <b>1a</b> | 58-306-L           | Armrestpad left  | <b>14</b> | 58-302                     | Bearing (x2) Cross section               |
| <b>1b</b> | 58-305             | Armrestpad center                                      | <b>15</b> | 58-353                     | Turn axle, beam                          |
| <b>1c</b> | 58-306-R           | Armrestpad right                                       | <b>16</b> | 57-776<br>57-775           | Cover, Wheel<br>Washer, wheel            |
| <b>2a</b> | 58-363             | Frame/Armrest center                                   | <b>17</b> | 58-360                     | Cover, Wheelplate (PA)                   |
| <b>2b</b> | 58-304-L/R         | Frame/Armrest center<br>(left/right)                   | <b>18</b> | 58-354                     | Wheel mount beam                         |
| <b>2c</b> | 57-352             | Lock lever   | <b>19</b> | 57-051<br>57-319<br>57-049 | Wheel 75mm<br>Wheel 100mm<br>Wheel 125mm |
| <b>2d</b> | 58-301             | Clamp aluminium  | <b>20</b> | 58-355-L<br>58-355-R       | Bottom beam, left<br>Bottom beam, right  |
| <b>3</b>  | 57-041-3           | Holder, Remotecontrol (TH7)                            | <b>21</b> |                            | Linking arm, right                       |
| <b>4</b>  | 58-376             | Battery, TiMotion                                      | <b>22</b> |                            | Linking arm, left                        |
| <b>5</b>  | 58-377             | Actuator, TiMotion                                     | <b>23</b> | 58-310-1                   | Hook (for knee support)                  |
| <b>6</b>  | 58-373<br>58-373-1 | Controlbox 220V, TiMotion<br>Controlbox 110V, TiMotion | <b>24</b> | 58-312                     | Knee support                             |
| <b>7</b>  | 58-351             | Vertical frame   | <b>25</b> | 58-385                     | Holder/Knee support (only PUR)           |
| <b>8</b>  | 58-311             | Telescopic Innertube<br>incl. bronze bearing           | <b>26</b> | 58-308-1-L/R               | Hinged arm/knee support<br>(left/right)  |
| <b>9</b>  | 58-358             | Sideplate (2x) alu                                     | <b>27</b> | 57-710                     | Knob, hook adustment L=27                |
| <b>10</b> | 58-356             | Aluprofile, widening                                   | <b>28</b> | 57-839                     | Knob, Hinged arm/knee, L=15              |
| <b>11</b> | 58-378             | Actuator, widening (TiMotion)                          | <b>29</b> | 58-302                     | Bushing, PA6                             |
| <b>12</b> | 58-364             | Circular plate   | <b>30</b> | 58-322                     | Strap blocker, green                     |
| <b>13</b> | 58-352             | Cross section  |           |                            |  |

## 2. Accessories

| Part no.  | Description                |
|-----------|----------------------------|
|           | Manual brake, 2 handles    |
|           | Manual brake, 1 handle     |
| 56-333-DB | Standing plate, Short      |
| 56-383-DB | Standing plate, Long       |
| 56-334    | Dripstand, Chromed         |
| 56-334    | Holder for Dripstand       |
| 56-336    | Oxygen tube holder         |
| 56-337    | Side support               |
| 56-338    | Dripstand holder, Complete |
| 56-387    | Wheel w brake 75 mm        |
| 56-358    | Wheel w brake 100 mm       |
| 56-361    | Wheel w brake 125 mm       |
| 57-365    | Armrestpad center, PUR     |

TECHNICAL MANUAL

|                     |                                   |
|---------------------|-----------------------------------|
| 57-365-L/R          | Armrestpad left/right, PUR        |
| 57-367              | Kneepad, PUR                      |
| 58-374-2            | Remote Control (TH7)              |
| 56-062              | Remote Control PLUS, DB (TH10)    |
| 58-320 (-1, -2, -3) | Cable/EUR (-UK, -US, -AUS)        |
| 58-326 (-1, -2, -3) | Coiled Cable/EUR (-UK, -US, -AUS) |

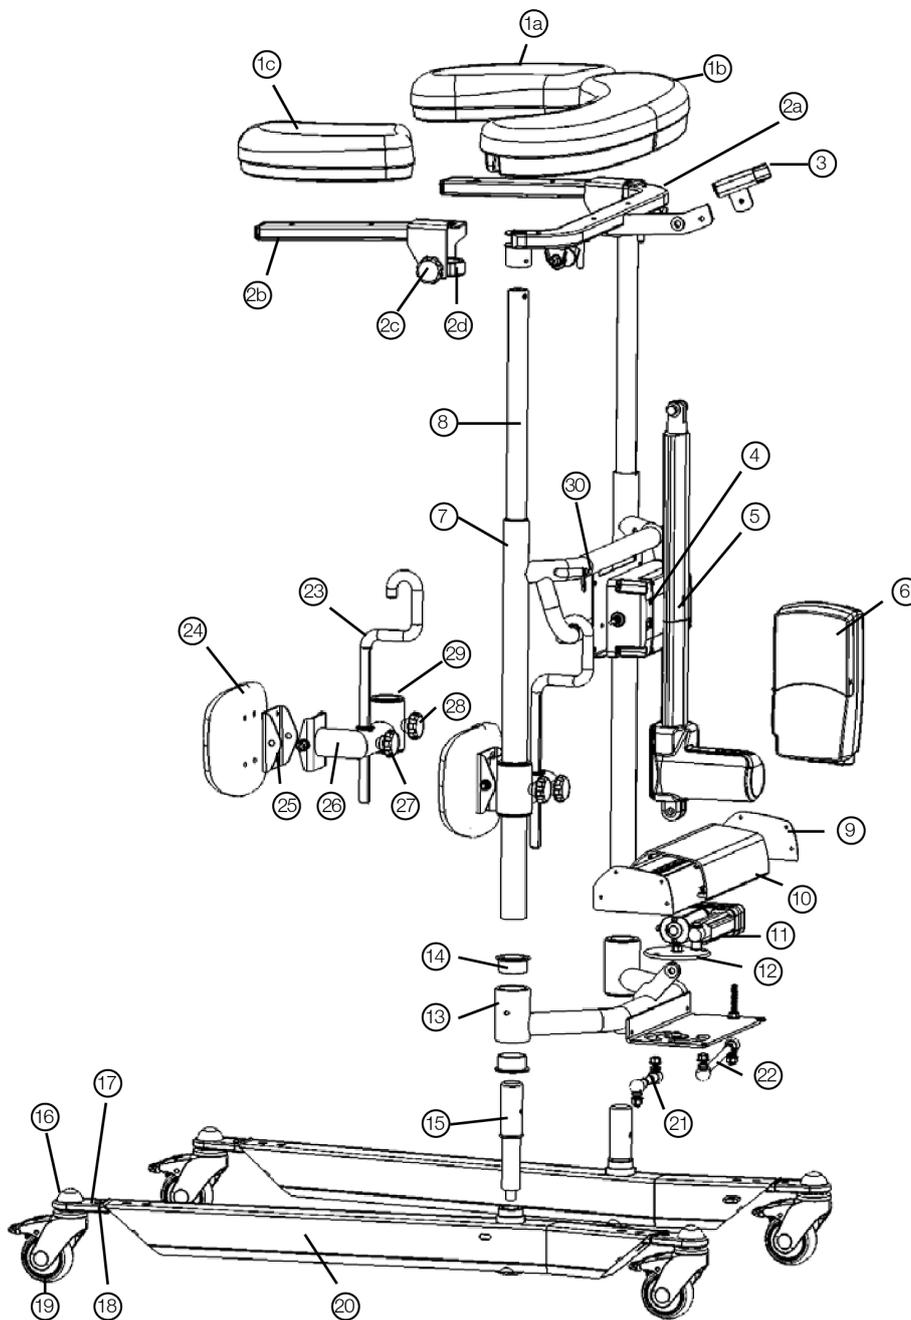

### 3. Electrical system – Technical data

| Actuator                 | Lift                 | Widening |
|--------------------------|----------------------|----------|
| Producer                 | T-Motion             | T-Motion |
| Voltage                  | 24V                  | 24V      |
| Push                     | 2000N                | 1000N    |
| Pull                     | 2000N                | 1000N    |
| Self-locking push        | 1000N                | 1000N    |
| Current                  | 4.6A                 | 2.8A     |
| Colour                   | Black                | Black    |
| Stroke                   | 400mm                | 55mm     |
| Mounting dim             | 605mm indragen längd | 167mm    |
| Encapsulation            | IP66                 | IP66     |
| IEC 60601-1 3rd revision |                      |          |

#### Controlbox + Battery

|                          |                            |
|--------------------------|----------------------------|
| Producer                 | T-Motion                   |
| Voltage                  | 24V                        |
| Capacity                 | 2.0AH                      |
| Encapsulation            | IP66                       |
| Colour                   | Svart                      |
| Electrical safety        | Class II (Dubbelisolering) |
| IEC 60601-1 3rd revision |                            |

### 4. Remote Control Plus

\*\*1. Service indicator – flashes red after 11 months' operation. Constant light (red) after 12 months' operation. The indicator is a reminder to review the maintenance instruction (see Instructions for Use/Technical Manual. This should be done at least once every 12 months.

Reset: hold down buttons <2a> + <2b> for at least 30 seconds.

\*\*The indicator will go out around 30 seconds after the remote control is activated (battery conservation function).



## 5. Control box wiring

Remove the control box cover to make the connections as described below. Use a screwdriver or similar; refer to the special labels on the control box.

NOTE: Make sure that plugs are connected to the correct sockets otherwise the actuators can be damaged.

1. Socket for the height adjustment actuator.
2. Socket for the width adjustment actuator.
3. Remote control socket.
4. Battery terminal socket.
5. Plug socket (NOTE: Plugs must ALWAYS be connected to the control box for IP classification to be valid).



## 6. Battery charging

- Connect plug to 230V wall socket. Charging begins automatically and the battery LED flashes green.
- Make sure the battery is fully charged before using for the first time. It takes around 25 h to fully charge the battery.
- We recommend that the battery plug be removed from the control box if the product will be out of use for an extended period (more than one week) or if the battery is switched off by means of the ON/OFF switch. This eliminates the risk of disabling the battery as the control box always uses a small quantity of electricity even when the walker is not in use.

## 7. LED on controlbox and battery

Control box – green light when power is available from battery/mains socket.

Battery:

- The LED flashes green during charging.
- ON/OFF: To use the product, press ON.
- The green lamp will begin to flash.
- Use the OFF button (hold down for 5 s) to switch off the battery if the product will not be used for an extended period.
- The LED will show a constant green light when the battery is fully charged.
- When the battery is in normal state/in operation, the LED flashes green at REGULAR intervals, namely 0.5 s ON, 4 s OFF.
- When the battery requires charging (remaining charge <25%) the LED will flash orange/red at REGULAR intervals, namely 0.5 s ON, 4 s OFF.



NOTE: The battery has an in-built device that automatically switches it off when remaining charge is <20%. The LED is then extinguished. The battery must now be fully charged before the electronics can be used again.

## 8. Maintenance

Recommended at least once per year.

### Check that

#### General

The walker feels firm/does not feel loose.  
The walker does not rattle during manoeuvres.  
The walker is level and all of its castors are in contact with the floor.  
The walker is not dirty.

### Action

Clean with lukewarm soap solution or alcohol-based cleaning agent (no petroleum products).

#### Arm rests

Arm rests are intact and clean.  
Arm rest widening is functional.

Clean; replace if damaged.  
Replace lock knob.

#### Handle

Grips are not damaged/dirty.  
Handle adjustment is functional.

Clean with lukewarm soap solution (no petroleum products).  
Replace handle grips.  
Fit lock knobs/plates as required.

#### Battery

Check that the charging cable is connected to the control box.  
Check that the remote control is connected to the control box.  
Connect or fit new remote control as required.  
Check that the battery, actuators and control box are not loose.

Fit new cable; this must always be connected to the control box (IP65 classification).  
Connect; replace with new remote control as required.  
Refer to the wiring diagram in the Technical manual.  
Tighten; replace with new fasteners as required.

#### Height/width adjustment

Raising and lowering are functional.  
The walker feels stable at maximum settings.  
There is no looseness between the vertical frame and bottom frame.  
Height adjustment clamps lock.  
The electric actuator must not feel loose.  
Height adjustment via remote control is functional.  
The electric actuator must run smoothly at a constant speed.

Fit new guide sleeves (in frame) or end plugs (in chrome tubes) as required.  
The technical manual shows the design and which fasteners must be checked. Contact the distributor if the parts cannot be tightened.  
Replace clamps.  
Tighten the attachment fitting concerned; replace bolts/ lock nuts as necessary.  
Check that the battery/remote control/actuator are connected in accordance with the wiring diagram.  
Charge the battery. Contact customer services.

#### Frame parts

There is no mechanical damage.  
There are no scratches.  
End plugs/lower frame fitted.

If damage is present, contact GATE's customer services.  
Touch up as necessary.  
Fit new end plugs.

**Castors/brakes**

Castors roll easily/tread not damaged.  
 The castors are tightly fastened to the lower frame.  
 Castor brakes functional on all castors.  
 Handbrake functional.

Clean or replace castors (NOTE! Castors are always fixed to the lower frame with thread locker or lock nuts. The castors are sealed and we do not recommend their dismantling; instead, replace the whole castor assembly.  
 Tighten the castor bolt and fit locking nut or use thread locker (depends on model).  
 Replace castor assembly.  
 Adjust the brake or fit new castors.

**Harness**

Belts, seams and Velcro fasteners are whole/intact.  
 The walker lockplate (green) is functional.

Replace harness. Available in three sizes (S, M, & L)  
 Replace lockplate

**Holder, belts**

Holder, belts not bent (see Figure s3).  
 Harness and attachment belts must be replaced every three years.

A bent holder is a sign that the product has been overloaded.  
 The frame must be replaced before further use.  
 The action is then "Check harness labeling. If the harness production date is older than 3 years, the harness and belts must be scrapped.

**9. General safety/maintenance advice**

The Bure Walker may only be used:

- As a WALKING AID / STAND-UP AID.
- INDOORS on HARD, LEVEL surfaces.


Before use, always check that:

- The product feels firm, secure and stable
- Harnesses, belts and attachments are intact and undamaged

Wipe the walker and its armrests clean as necessary; use soap solution/surface disinfectant. Be aware of battery charge status (LED) – charge as necessary.

**10. ID label**

1. Part number
2. Product name
3. Date of manufacture
4. Max user weight
5. Serial number
6. EAN code

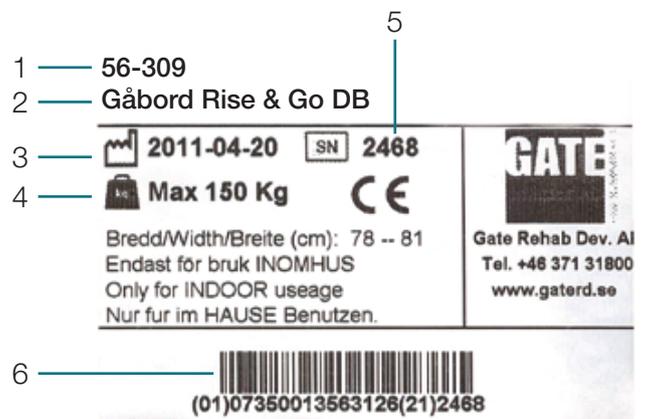

## 11. Recycling/Scrapping

When the product is no longer usable it should be recycled in accordance with legislation and regulations in the country concerned. All electrical parts including batteries must be removed and recycled as electrical components. (Ask your local recycling station for further information about how the different materials in the product (metals, plastics, electronics) should be recycled).

## 12. Warranty

We provide two years' warranty for manufacturing faults (does not apply to wear parts). For further information or enquiries please contact:

Gate Rehab Development AB  
 Industrigatan 2, S-330 21 Reftele  
 tel 0371-318 00  
 info@gaterd.se




A DIRECT HEALTHCARE GROUP COMPANY

## 13. Technical specifications

Dimensions apply to walkers with 125 mm castors.

| Part no. | Produkt width | Max user weight | Length | Height   | Weight | Armrest/Internal dimension |
|----------|---------------|-----------------|--------|----------|--------|----------------------------|
| 56-309   | 66-106cm      | 150kg           | 101cm  | 95-135cm | 40kg   | 34-65cm                    |

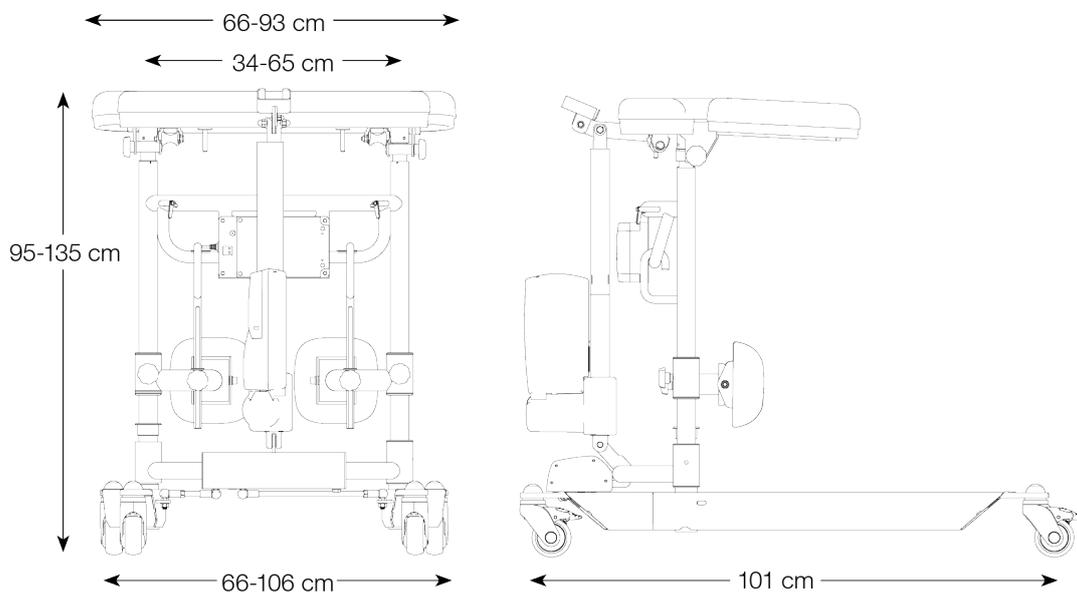





A DIRECT HEALTHCARE GROUP COMPANY

Gate Rehab Development AB  
Industrigatan 2  
Reftele, Sverige  
S-330 21

T: 0371-318 00  
F: 0371-318 01  
E: [info@gaterd.se](mailto:info@gaterd.se)

LIT-00107 Issue 1  
Date: January 2020

[GATERD.SE](http://GATERD.SE)